


012669 SVC-3 Voltammetry cell

After receiving the product, please check the contents.

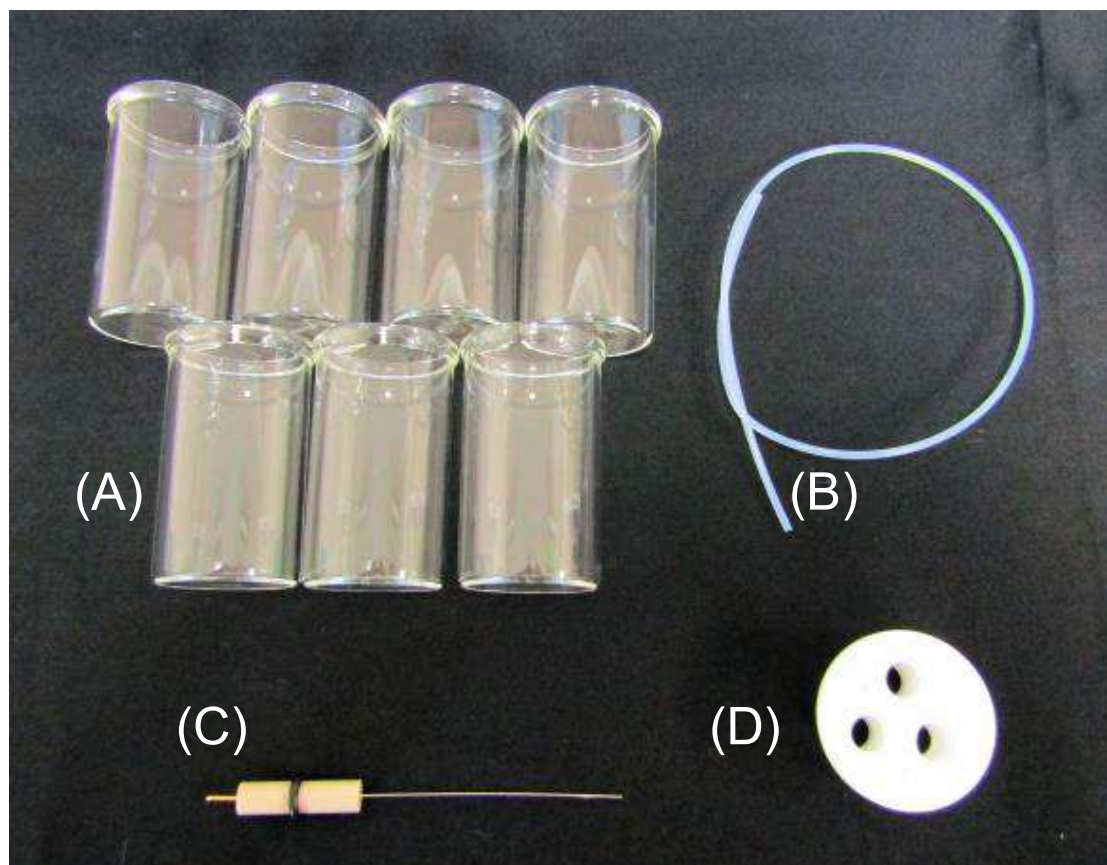

Contents

(A) Sample vial (20 mL)	7 pcs
(B) Purge tube	30 cm
(C) Platinum counter electrode 5cm	1 pc
(D) Teflon cap for SVC-3	1 pc

You can use the electrodes under dia 6mm (working, reference, counter electrode) for this product.

Please wash the vial thoroughly before experiment.

Any occurrence of damage after use is out of our guarantee.

Optional products

002012 GCE Glassy carbon electrode OD:6mm ID:3mm

012167 RE-1B Reference electrode (Ag/AgCl)

BAS Inc.

<https://www.als-japan.com> email: sales@als-japan.com